


## CONTRACTOR HCV TESTING/REPORTING

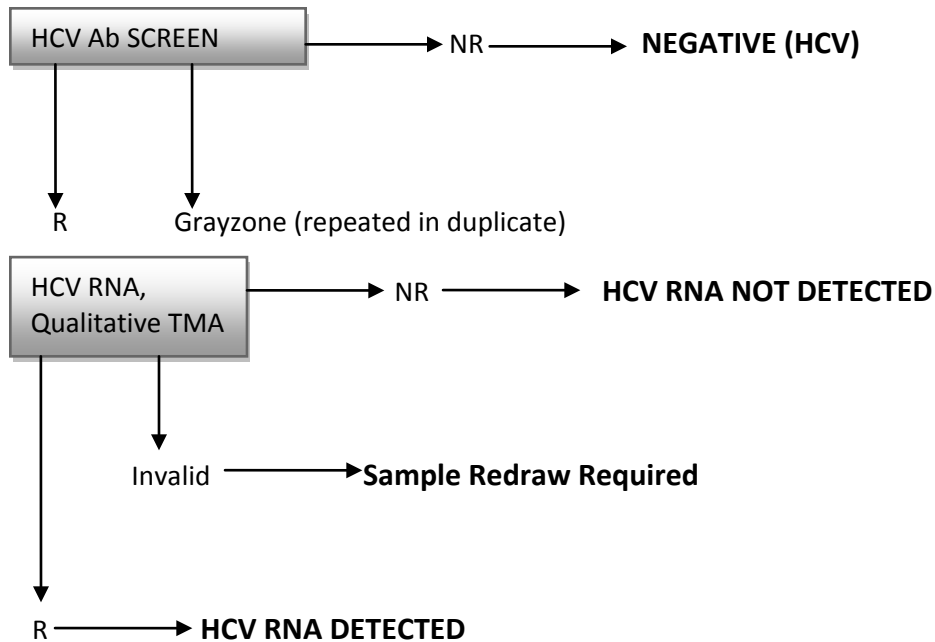

### VERSANT HCV RNA, Qualitative TMA Interpretation:

NR = HCV RNA was not detected. It does not preclude the presence of HCV RNA because results are dependent on adequate specimen collection, absence of inhibitors, and sufficient RNA to be detected.

R = HCV RNA was detected

Invalid = the sample must be retested. If the same result is generated the interpretation remains "invalid".

Results from the VERSANT HCV RNA Qualitative Assay should be interpreted in conjunction with other laboratory and clinical data available to the clinician.